

Fig. 1

1/6

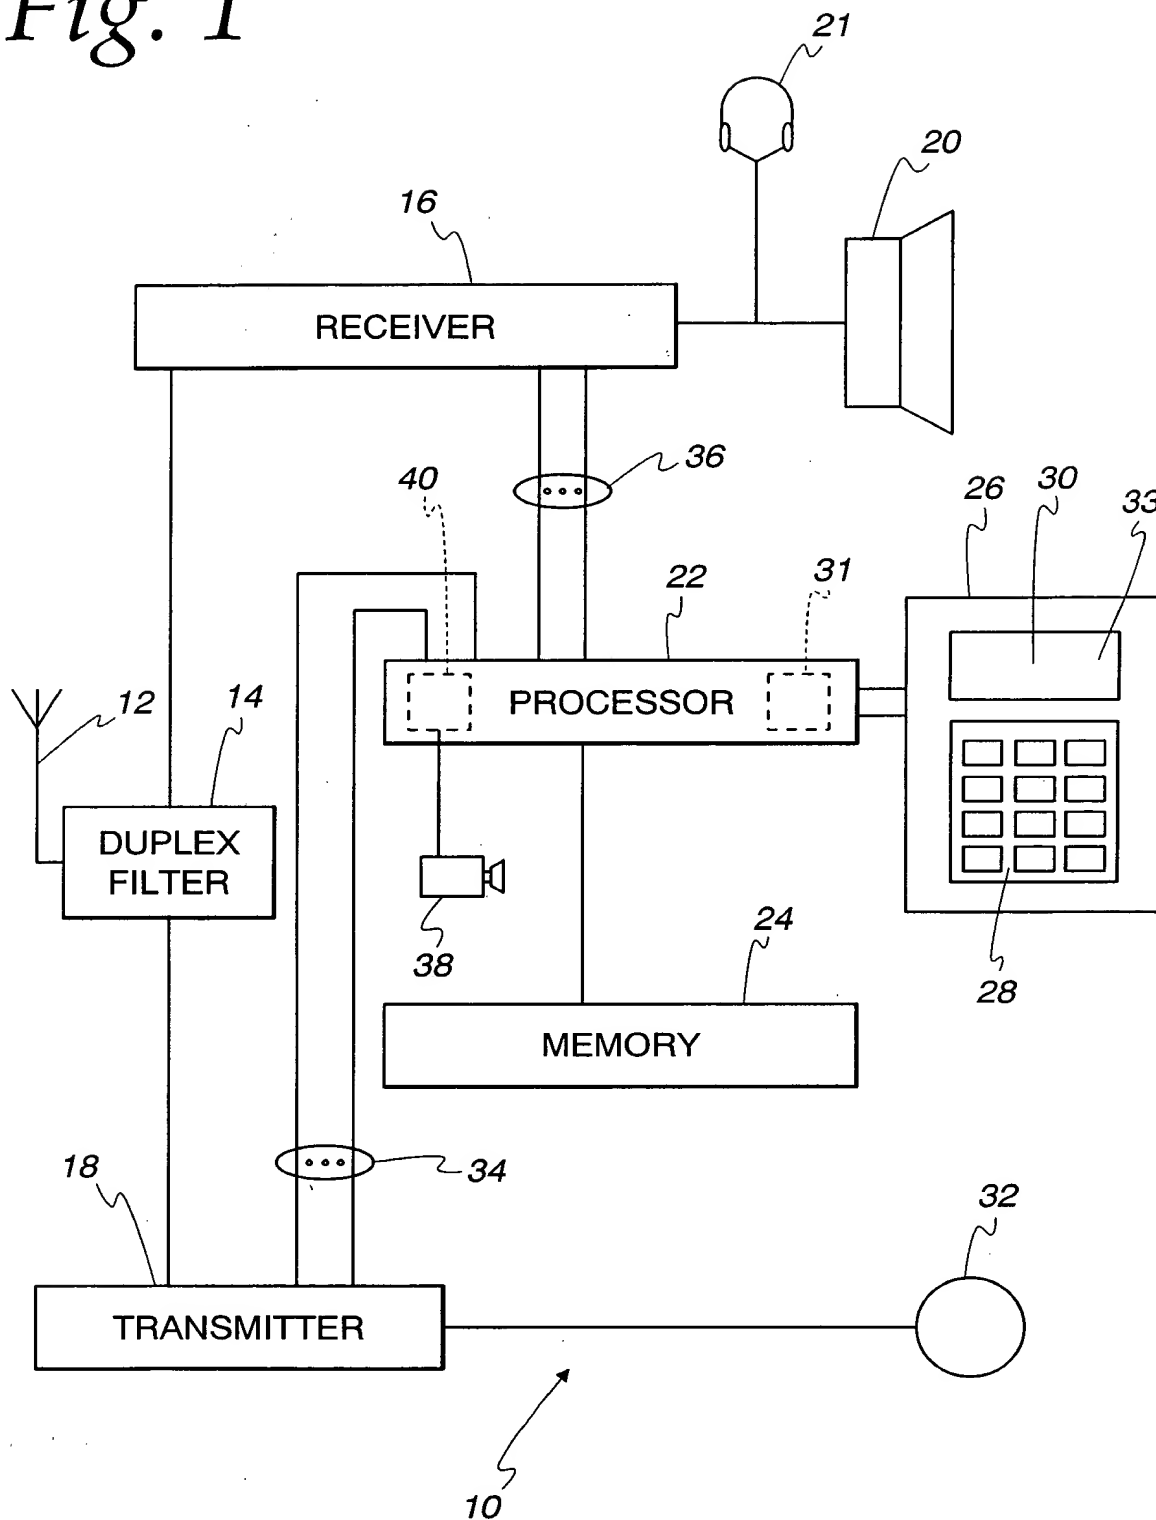




Fig. 2


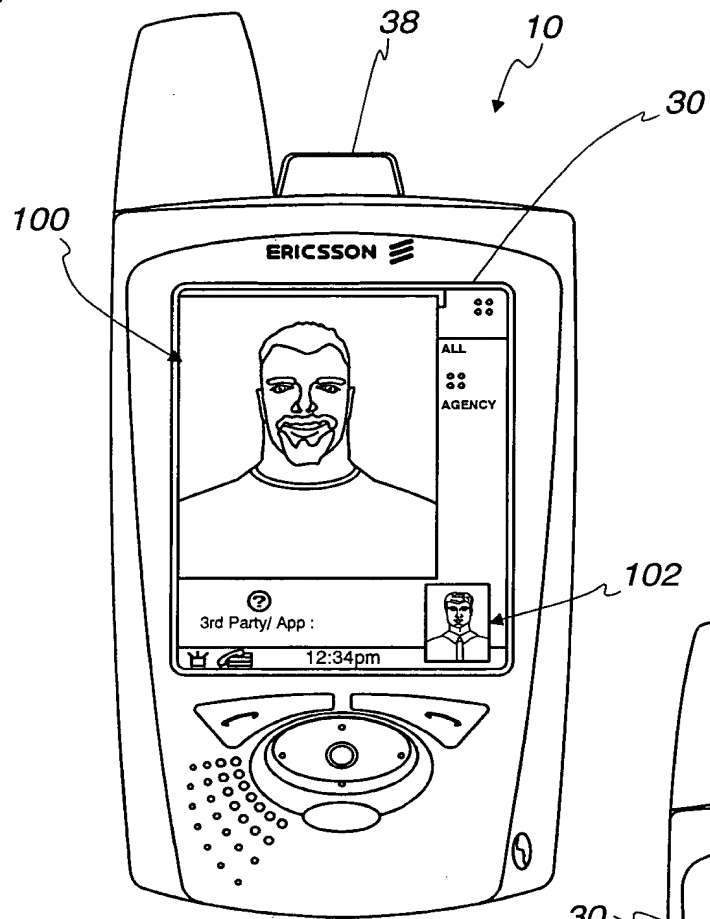


Fig. 3



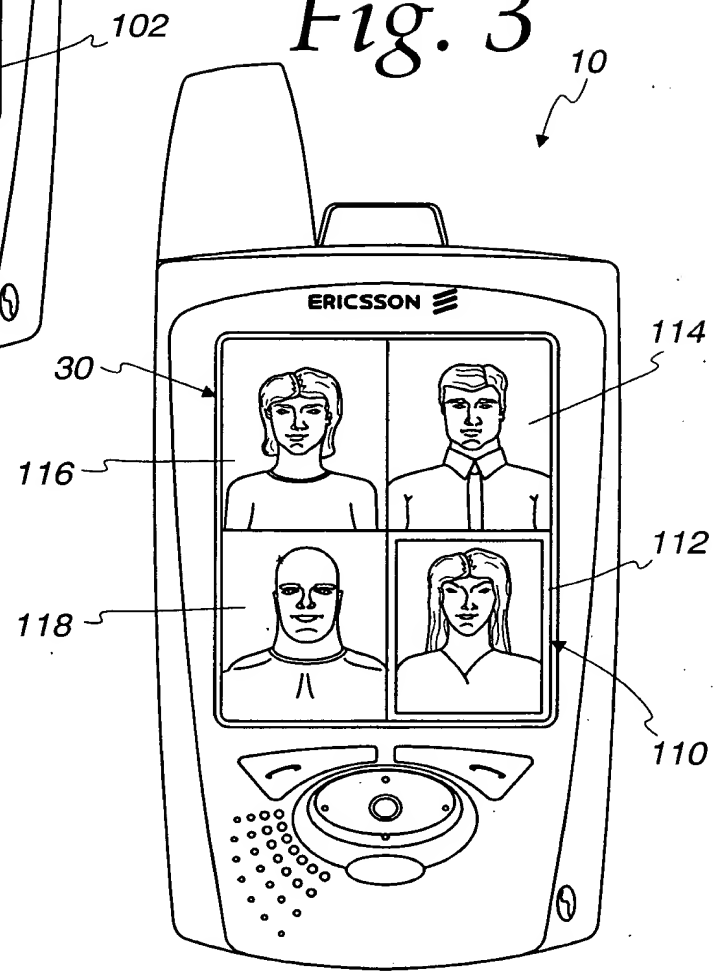

3/6

Fig 4


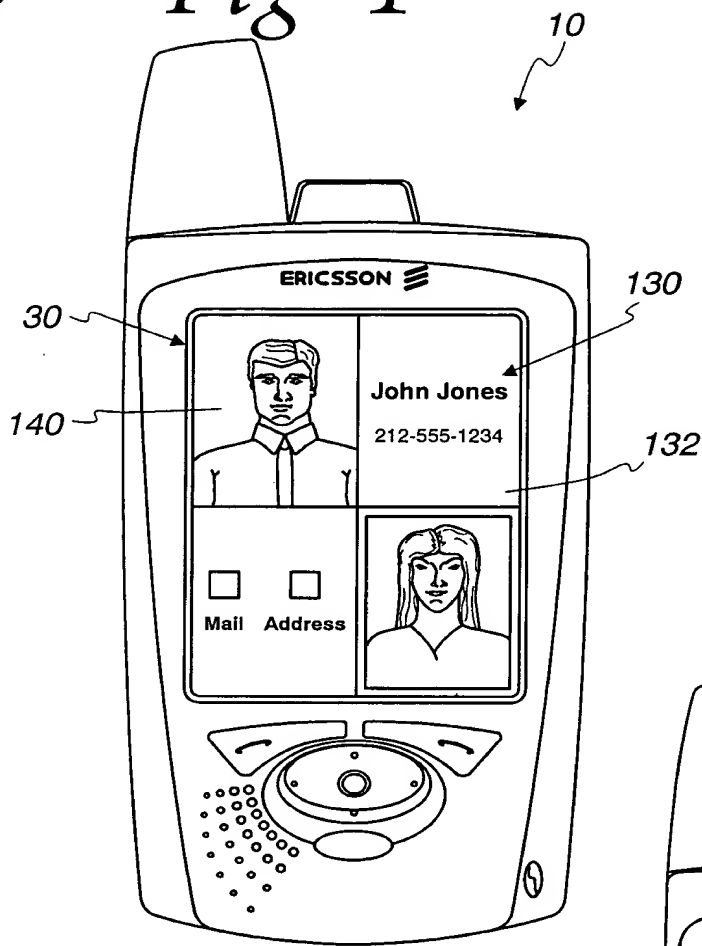


Fig. 5



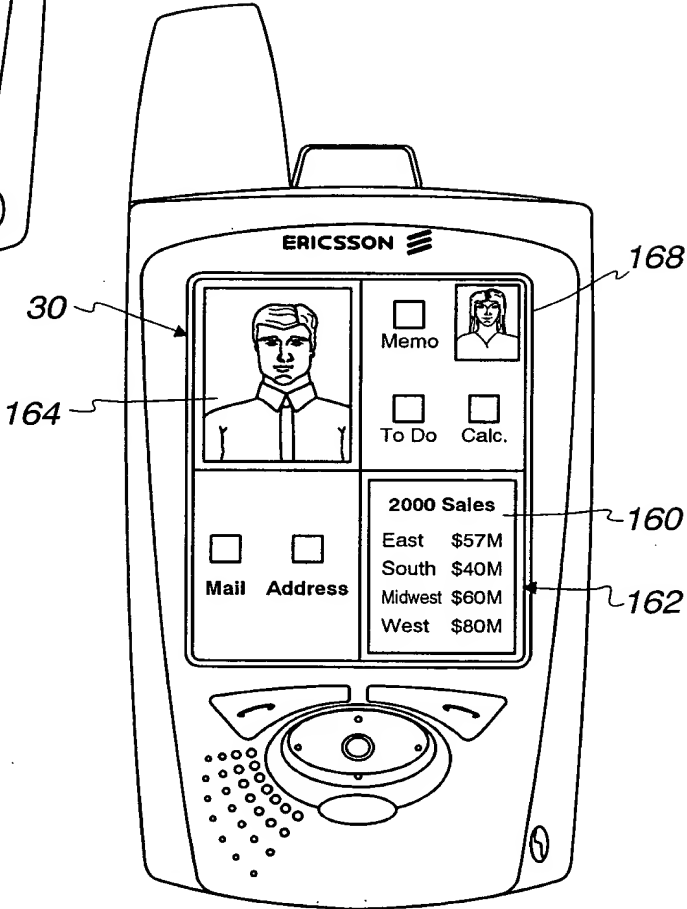

4/6

Fig. 6

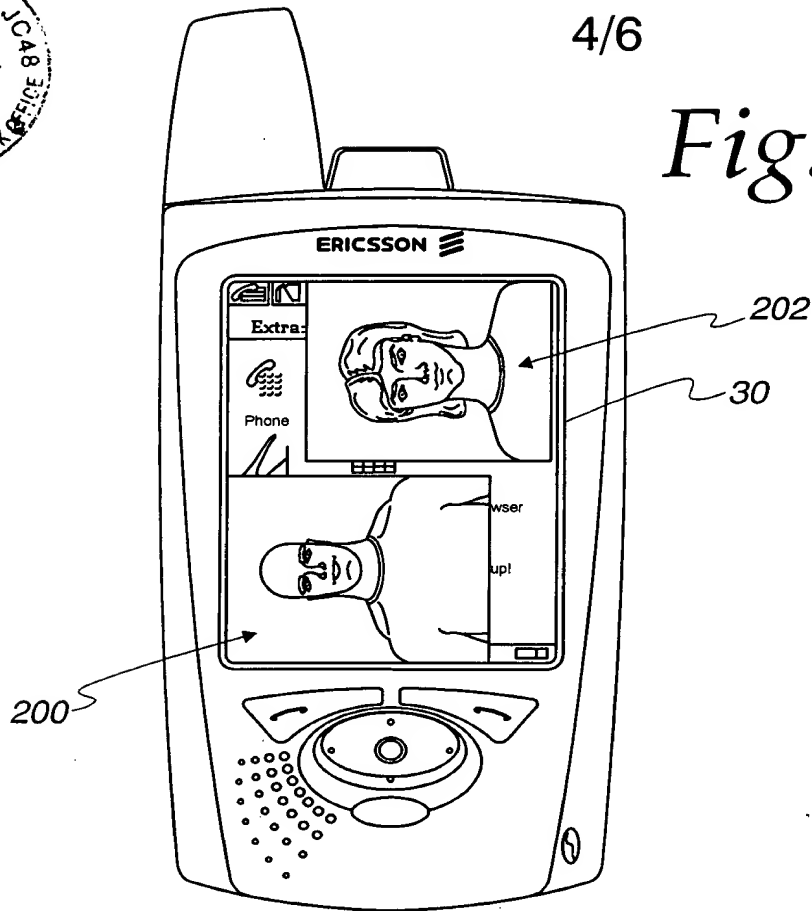
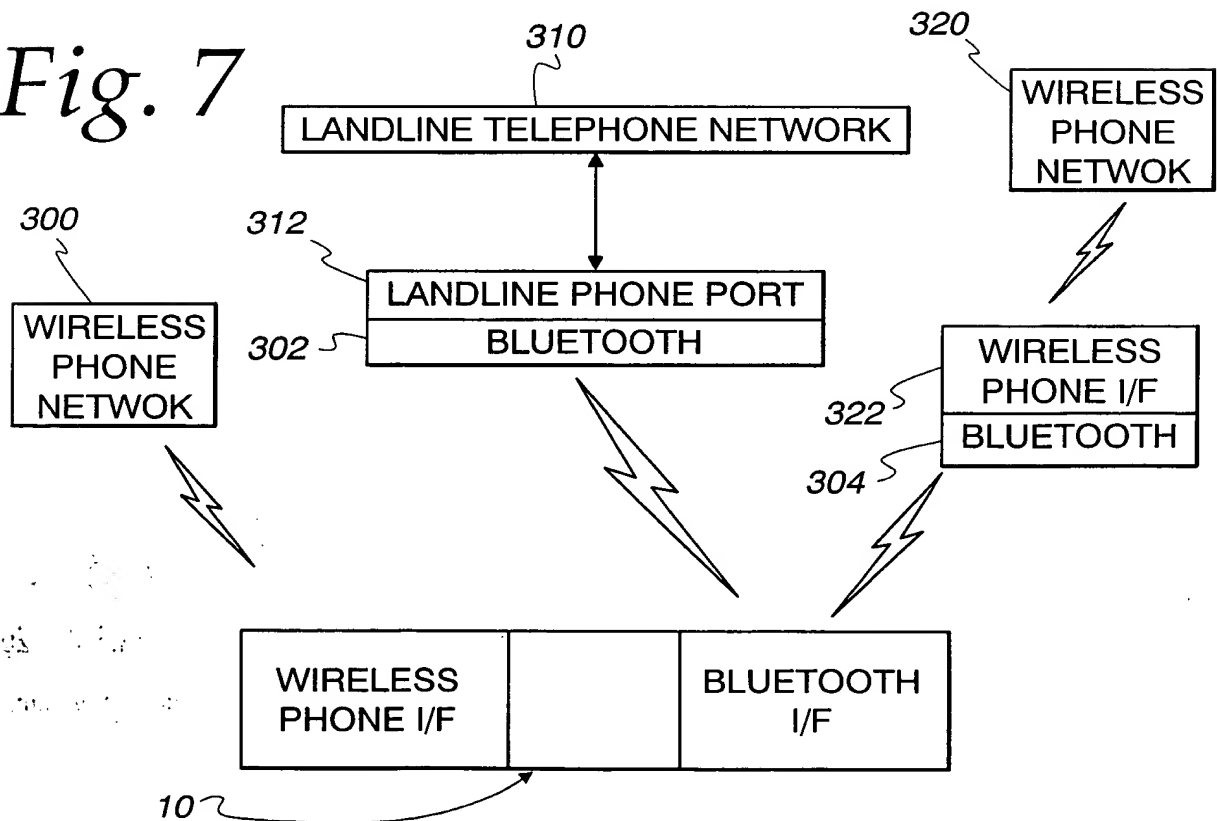


Fig. 7





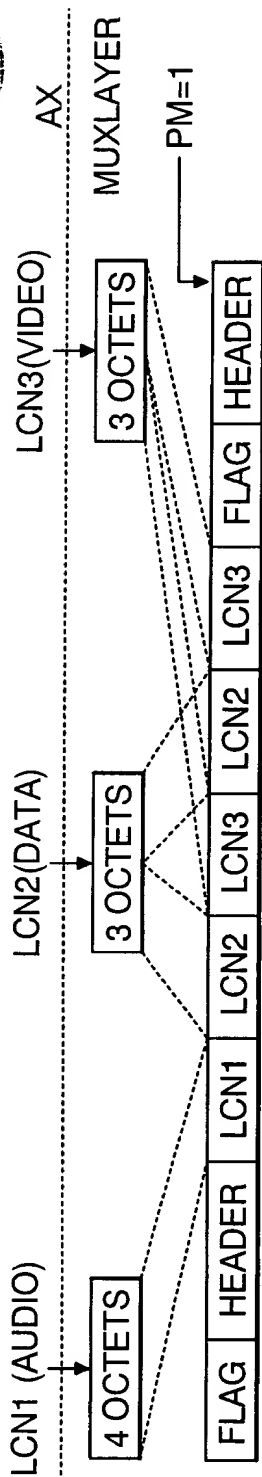


Fig. 8

Fig. 9

SCOPE OF RECOMMENDATION H.324



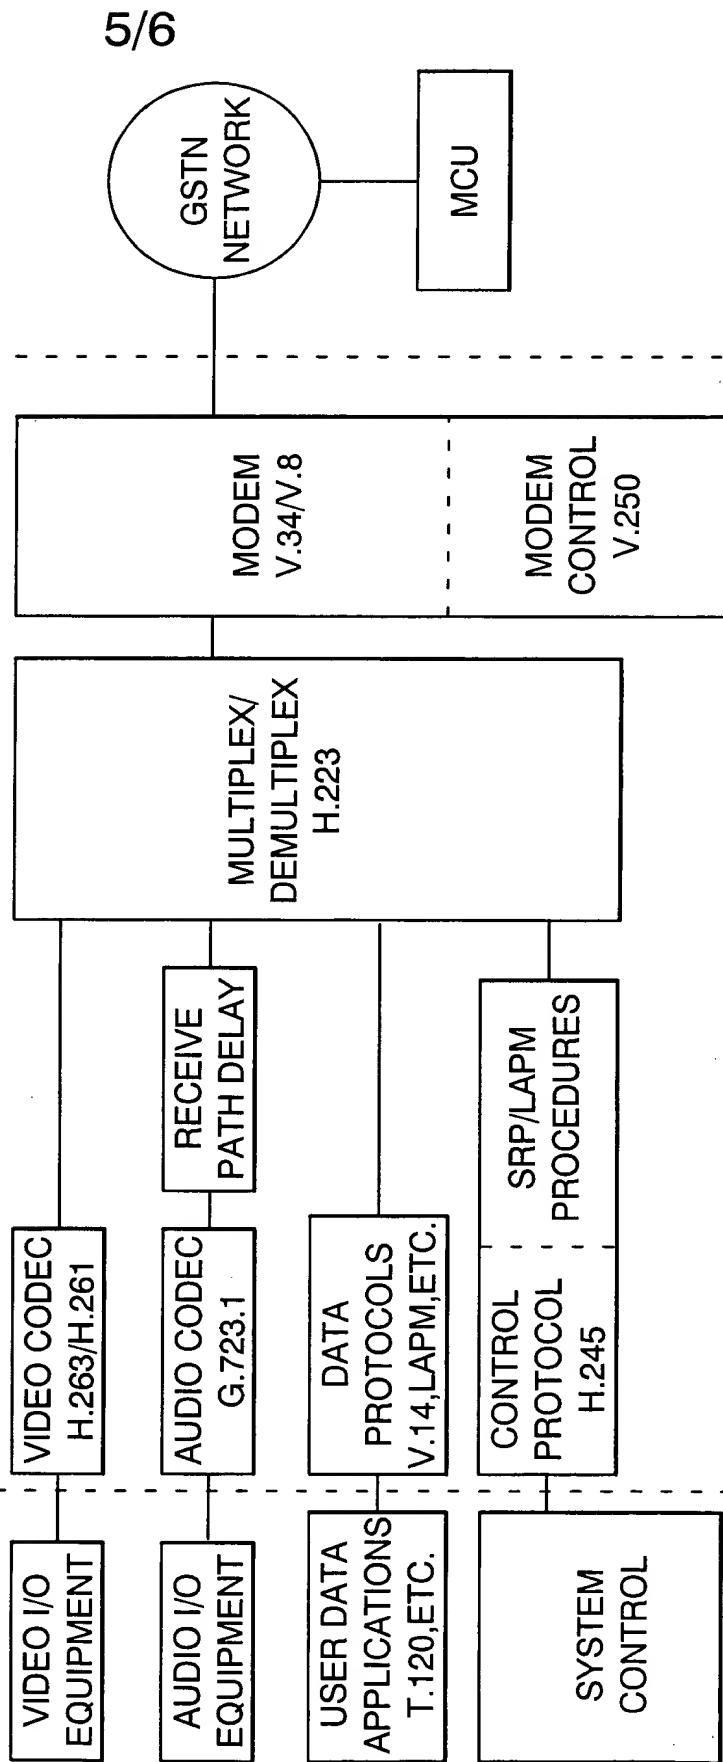

6/6

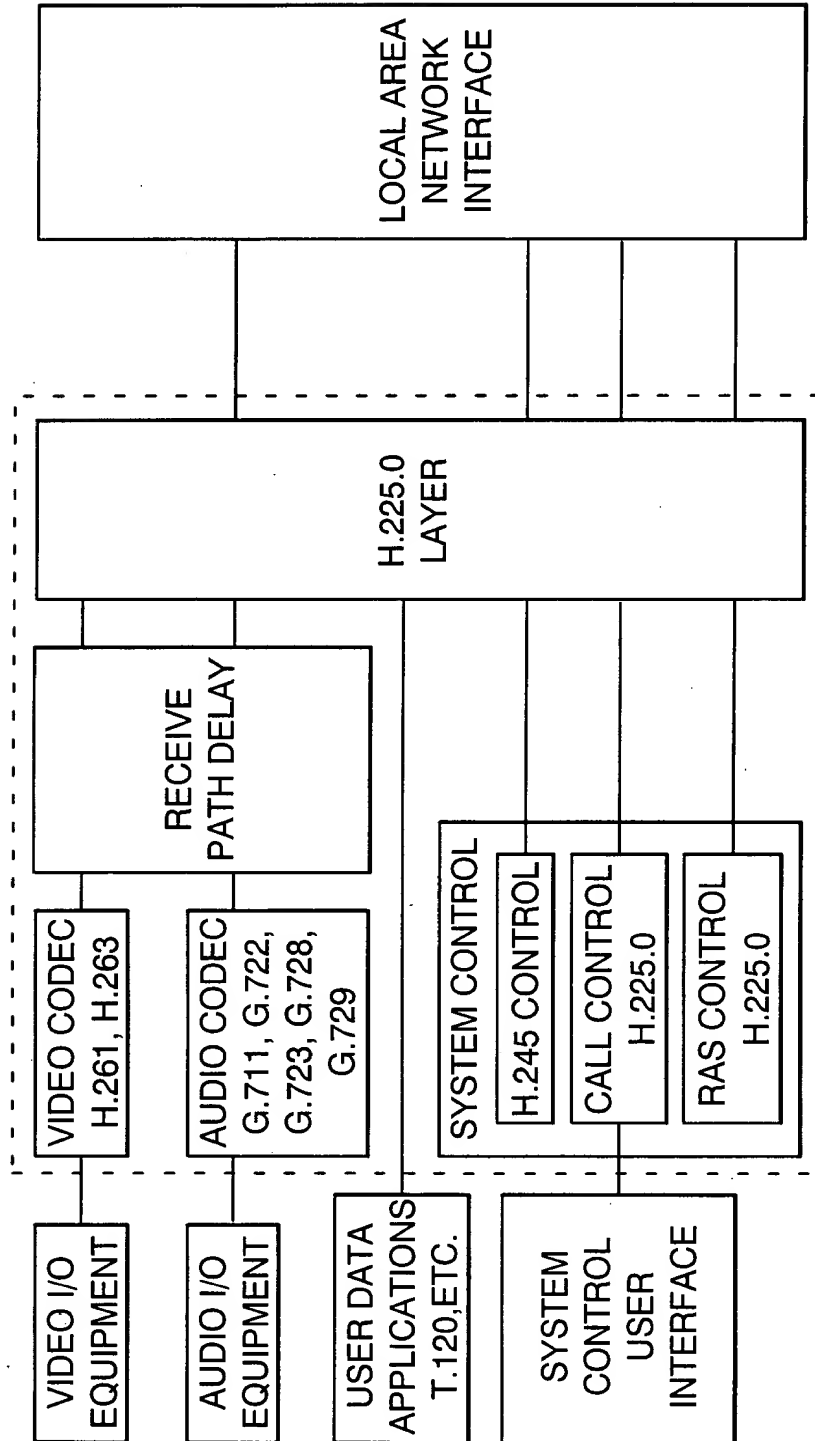


Fig. 10